

Soil Analysis

Submitted by **8888888**
AgSource Test Account
300 Speedway Circle, Unit 2
Lincoln, NE 68502

Submitted for
AgSource HARRISTURFELITE



Laboratory Sample #
DG27672 - DG27679
 Information Sheet #
TEST_20200923

Date Received
1-Jan-2026

Date Reported
03-Jan-2026

Field
TESTFIELD 1

Sample Identification	Phosphorus			Potassium	Calcium	Magnesium	Zinc	Manganese	Copper	Iron
	Bray I	Olsen	Mehlich							
	ppm	ppm	ppm	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Test13	73			73	862	116	2.9	0.7	4.7	99.8
Test14	51			55	789	114	2.3	0.5	4.2	67.3
Test15	68			67	881	114	4.2	1.5	5.8	136.1
Test16	55			67	900	120	3.4	1.4	5.4	89.2
Test17	22			57	883	191	3.3	0.9	2.5	72.9
Test18	19			66	791	201	0.9	0.6	1.0	32.6
Test19	13			49	793	196	1.9	0.6	0.9	48.0
Test20	11			47	921	158	1.2	0.3	1.4	43.7
Optimum Levels Greens	25 - 45			125 - 150	747 - 862	140 - 250	1.0 - 3.0	5.0 - 15.0	0.5 - 1.5	4.0 - 20.0

Sample Identification	Soil pH	Sodium	Soluble Salts	Organic Matter	Cation Exchange	Percent Base Saturation				
						Hydrogen	Sodium	Potassium	Calcium	Magnesium
		ppm	mmhos/cm	%	meq/100g	%	%	%	%	%
Test13	6.5	65.0	0.2	1.9	5.7		4.9	3.2	75.0	16.9
Test14	6.4	57.0	0.2	1.5	6.0	12.4	4.1	2.3	65.3	15.8
Test15	6.1	66.0	0.4	1.8	6.8	14.4	4.2	2.5	64.8	14.0
Test16	6.6	71.0	0.2	1.9	6.0		5.1	2.9	75.2	16.7
Test17	6.3	49.0	0.2	2.2	7.7	17.7	2.8	1.9	57.1	20.6
Test18	6.3	59.0	0.2	1.3	7.0	13.6	3.7	2.4	56.5	23.9
Test19	6.8	78.0	0.2	2.6	6.1		5.6	2.1	65.4	26.9
Test20	6.7	63.0	0.2	1.6	6.3		4.3	1.9	73.0	20.8
Optimum Levels Greens	5.9 - 6.5	20 - 120	0.1 - 1.0	1.0 - 3.0		< 5.0	2.0 - 7.0	65 - 75	15 - 25	

Sample Identification	Boron	Sulfur	Nitrate	Ammonium	Chloride	Aluminum	Particle Size Analysis			
							Sand	Silt	Clay	Soil Texture
	ppm	ppm	ppm	ppm	ppm	ppm	%	%	%	
Test13	0.2	19.9	5.5							
Test14	0.1	26.0	3.7							
Test15	0.2	72.9	4.0							
Test16	0.2	15.3	5.6							
Test17	0.1	8.2	9.7							
Test18	0.1	5.3	21.1							
Test19	0.1	5.7	8.9							
Test20	0.1	17.6	12.4							
Optimum Levels Greens	0.5 - 1.0	8.0 - 20.0	5.0 - 25.0							

DISCLAIMER: Data and information in this report are intended solely for the individual(s) for whom samples were submitted. Reproduction of this report must be in its entirety. Levels listed are guidelines only. Data was reported based on standard laboratory procedures and deviations.

Soil Analysis

Submitted by **8888888**
AgSource Test Account
300 Speedway Circle, Unit 2
Lincoln, NE 68502

Submitted for
AgSource HARRISTURFELITE




Laboratory Sample #
DG27672 - DG27679
 Information Sheet #
TEST_20200923

Date Received
1-Jan-2026

Date Reported
03-Jan-2026

Field
TESTFIELD 1

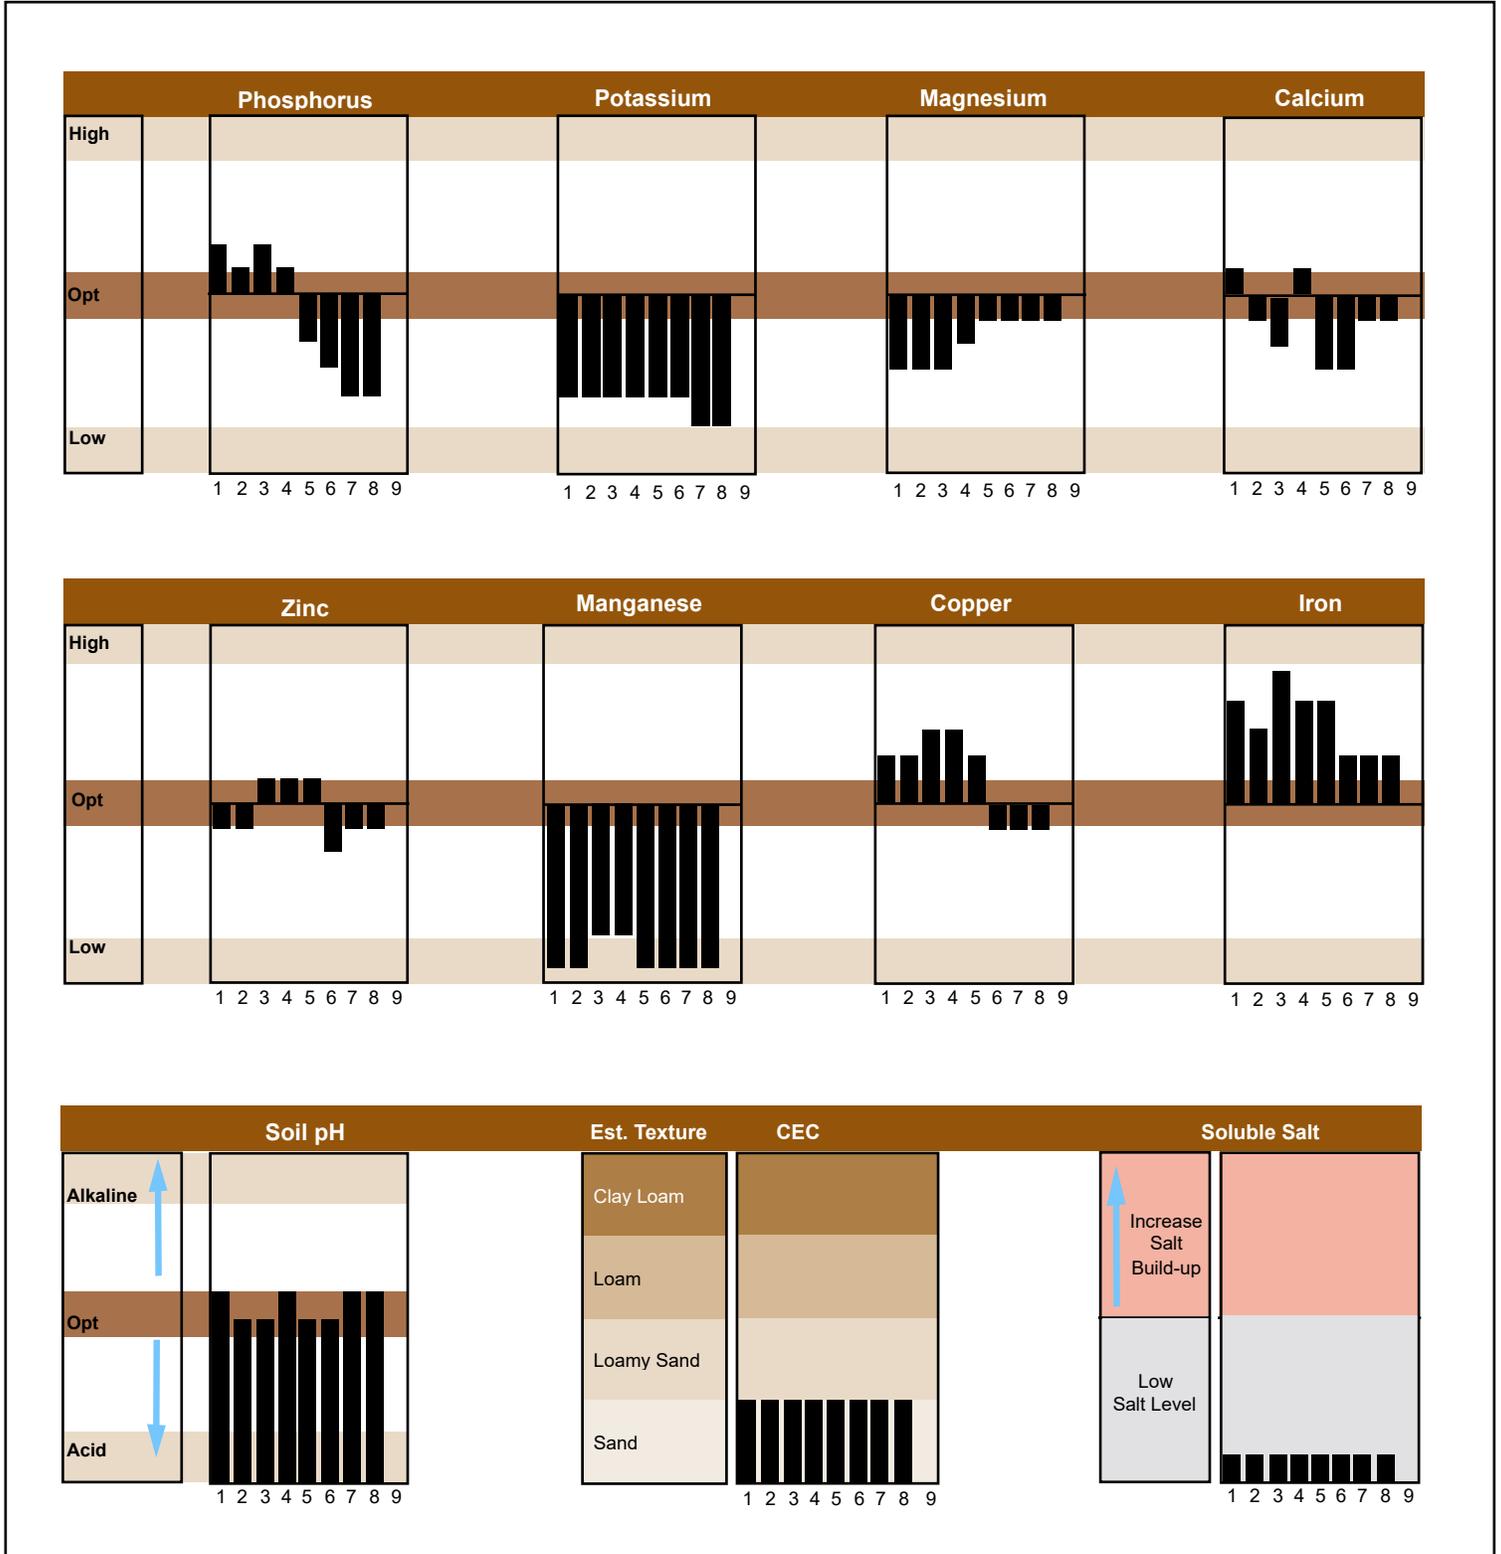

DISCLAIMER: Data and information in this report are intended solely for the individual(s) for whom samples were submitted. Reproduction of this report must be in its entirety. Levels listed are guidelines only. Data was reported based on standard laboratory procedures and deviations.

Soil Analysis



Submitted by **8888888**
AgSource Test Account
300 Speedway Circle, Unit 2
Lincoln, NE 68502

Submitted for
AgSource HARRISTURFELITE

Laboratory Sample #
DG27672 - DG27679
 Information Sheet #
TEST_20200923

Date Received
1-Jan-2026

Date Reported
03-Jan-2026

Field
TESTFIELD 1

Product Recommendation is Lbs./1,000 Square Feet

Sample Identification	Nitrogen N	Phosphorus P2O5	Potassium K2O	Magnesium Mg	Soil Amendment application			
					Limestone	Gypsum	Sulfur	Epsom
Test13	3.9	0.0	4.2	0.3	0.0	0.0	0.0	0.0
Test14	4.1	0.0	4.4	0.3	0.0	0.0	0.0	0.0
Test15	4.0	0.0	4.3	0.3	0.0	0.0	0.0	0.0
Test16	3.9	0.0	4.2	0.3	0.0	0.0	0.0	0.0
Test17	3.6	1.5	4.4	0.0	0.0	7.4	0.0	0.0
Test18	3.3	1.8	4.3	0.0	0.0	11.9	0.0	0.0
Test19	3.6	2.5	4.4	0.0	0.0	11.9	0.0	0.0
Test20	3.6	2.7	4.5	0.0	0.0	0.0	0.0	0.0

Plant food recommendations are for the entire growing season being presently grown.

Do not apply more than 1.0 lb/1,000 sf of Nitrogen any one application, if slow release N is used, more N can be applied, but no more than 3.0 lb/1,000 sf.

Product Recommendation is Lbs./Acre

Sample Identification	Zinc Zn	Manganese Mn	Copper Cu	Iron Fe	Sulfur S	Boron B
Test13	0.0	0.1	0.0	0.0	0.0	0.0
Test14	0.0	0.1	0.0	0.0	0.0	0.0
Test15	0.0	0.1	0.0	0.0	0.0	0.0
Test16	0.0	0.1	0.0	0.0	0.0	0.0
Test17	0.0	0.1	0.0	0.0	0.3	0.0
Test18	0.1	0.1	0.0	0.0	0.3	0.0
Test19	0.0	0.1	0.0	0.0	0.3	0.0
Test20	0.1	0.1	0.0	0.0	0.0	0.0